

Figure 1

Inhibiting Areola Test:


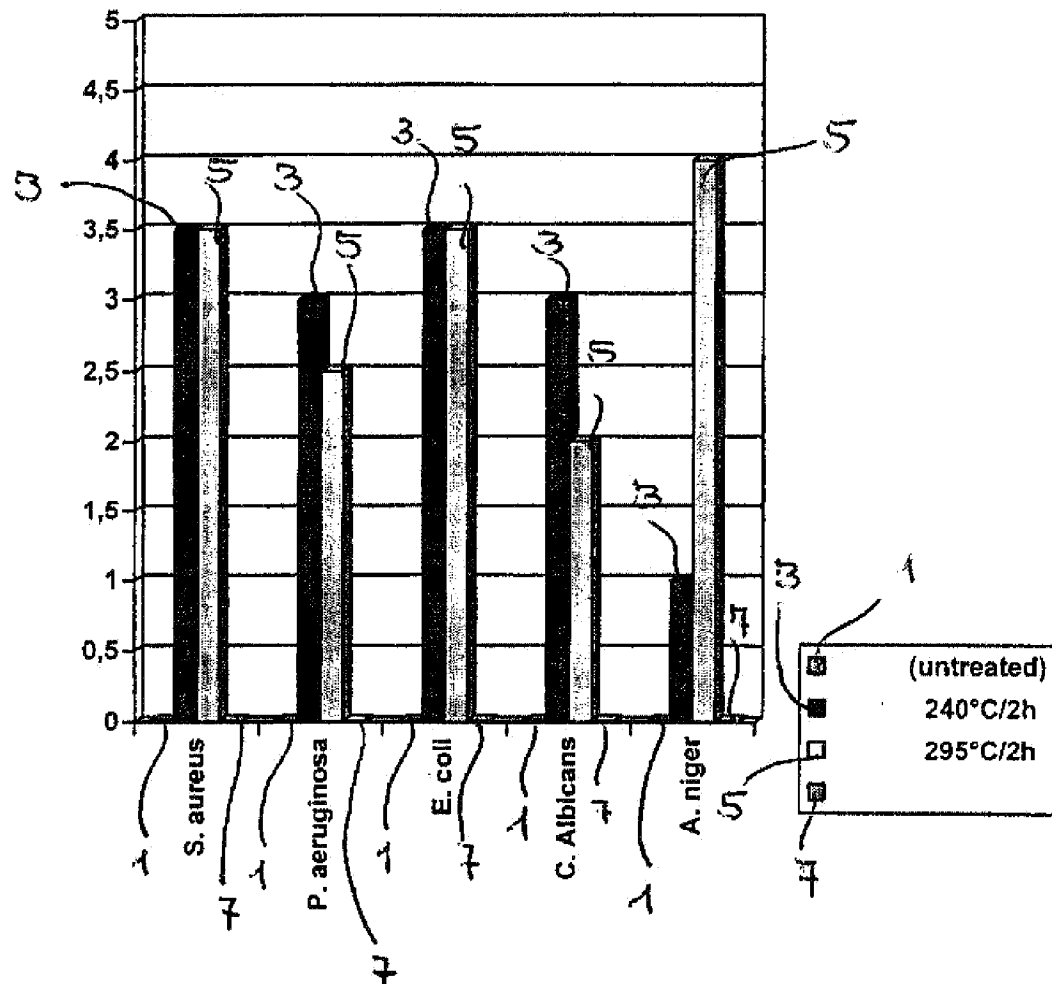


Figure 2

EMP (electron microprobe analyzer) Depth Profile, Concentration Profile Ag and Na

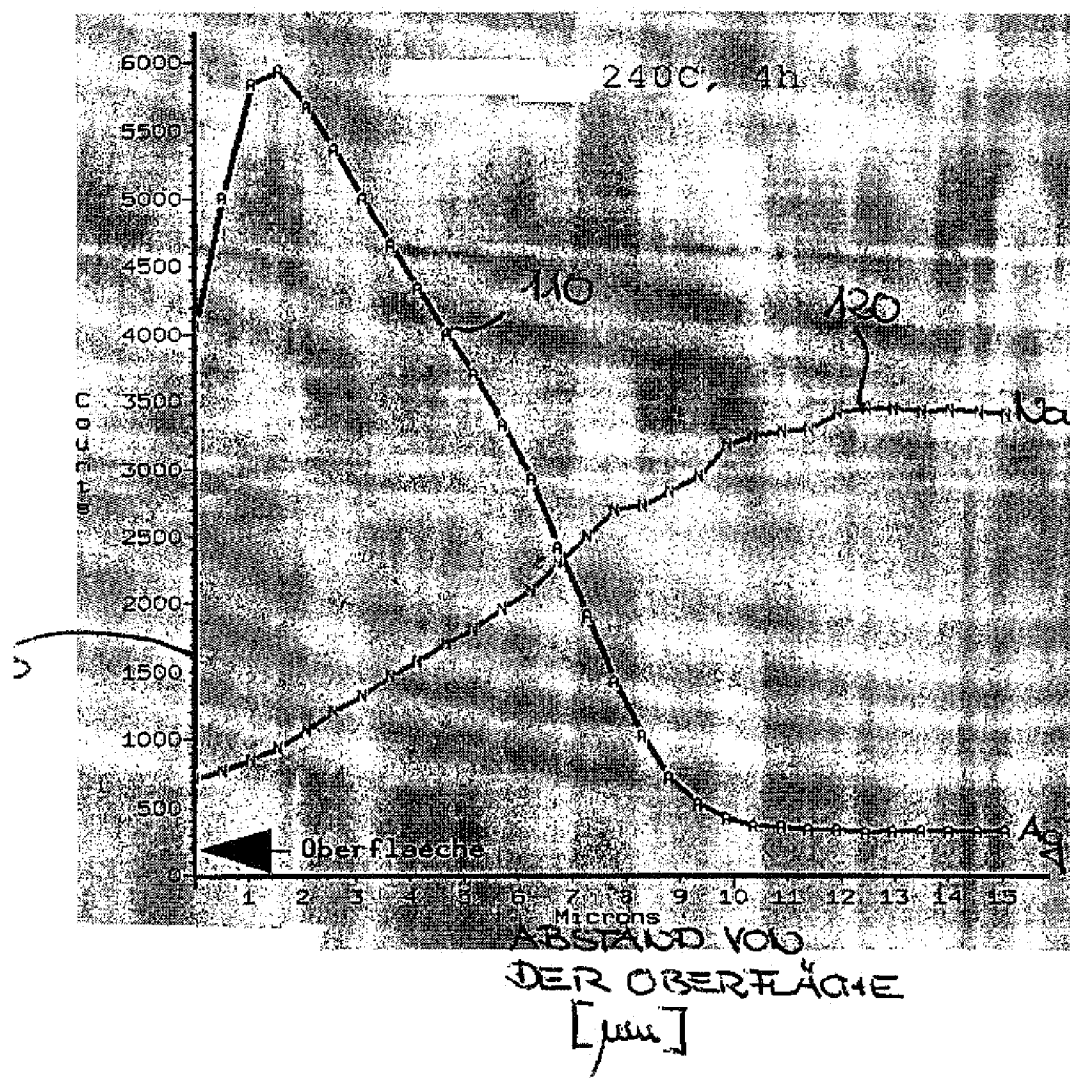

Oberfläche = Surface

ABSTAND VON = DISTANCE FROM

DER OBERFLÄCHE = THE SURFACE

Figure 3

Inhibiting Areola Test:

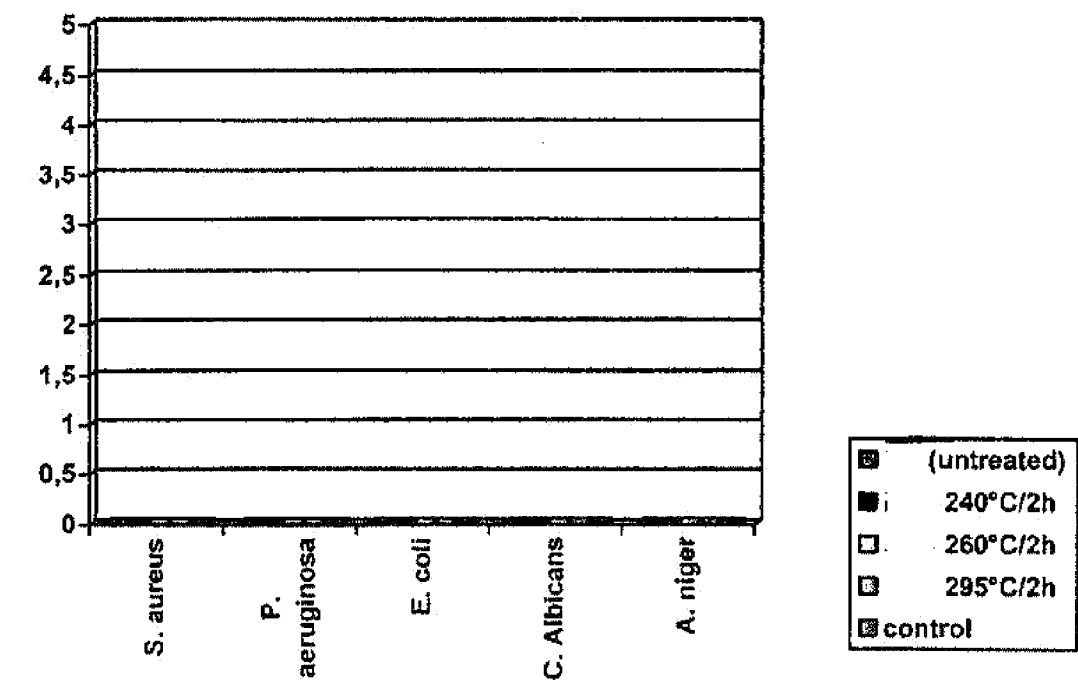


Figure 4

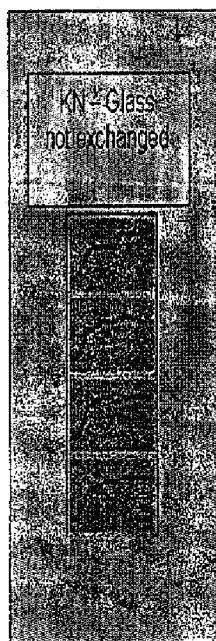


Figure 4a

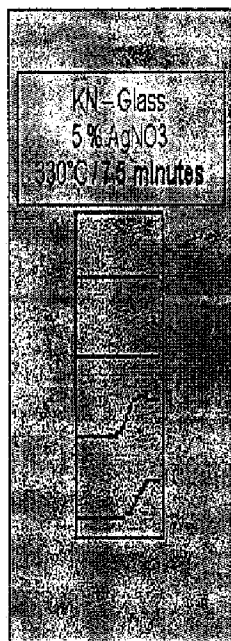


Figure 4b

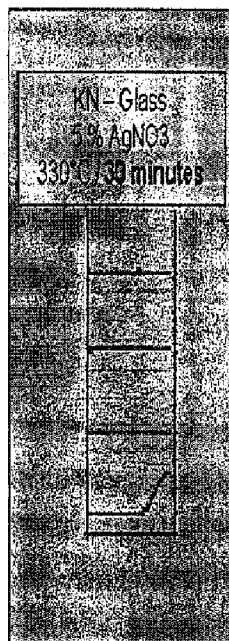



Figure 4c



Figure 4d

Figure 5

EMP (electron microprobe analyzer) Line Profile, Concentration Profile Ag and Na (Emb. 2)

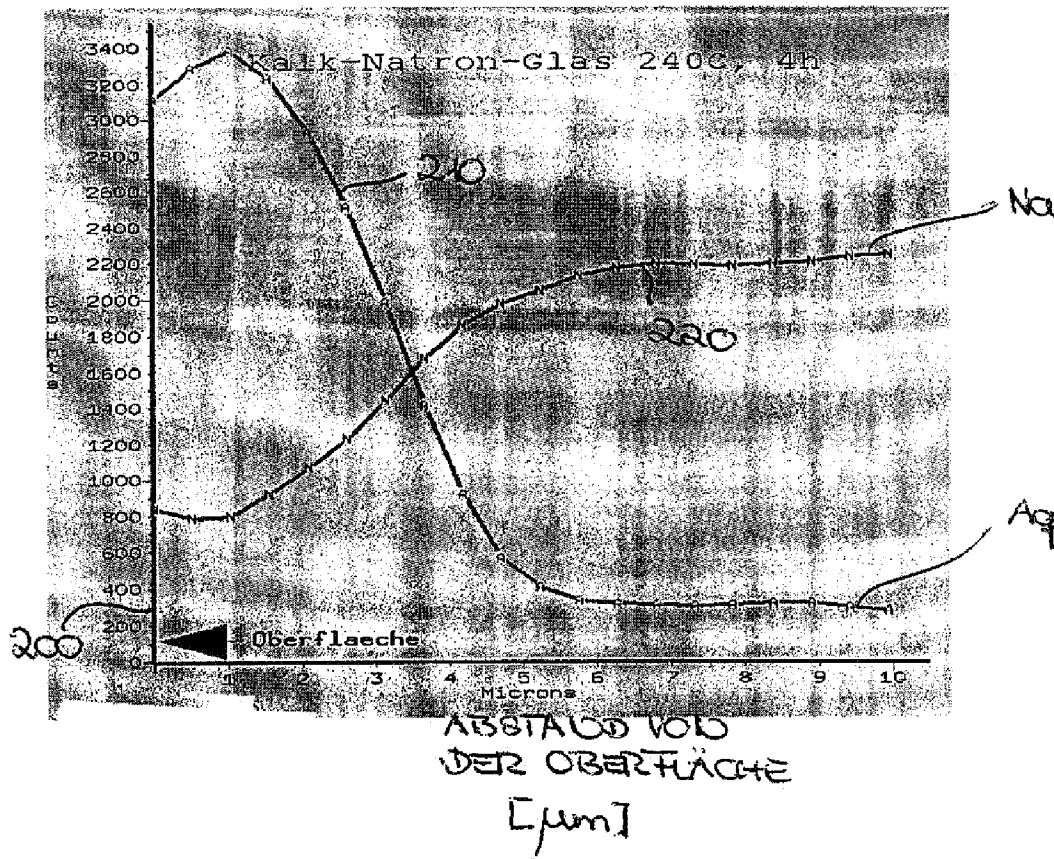

Kalk-Natron-Glas = Lime-Soda Glass

Oberfläche = Surface

ABSTAND VON = DISTANCE FROM
DER OBERFLÄCHE = THE SURFACE

